Onli

Ready for Use Hydrophilic Intermittent Catheter




You can be assured this intermittent catheter, which your clinician has recommended, has the features to help you catheterize with ease and comfort.

1 **Easy open packaging**

2 **Ready to use**

3 **Smooth hydrophilic coating for easy insertion**

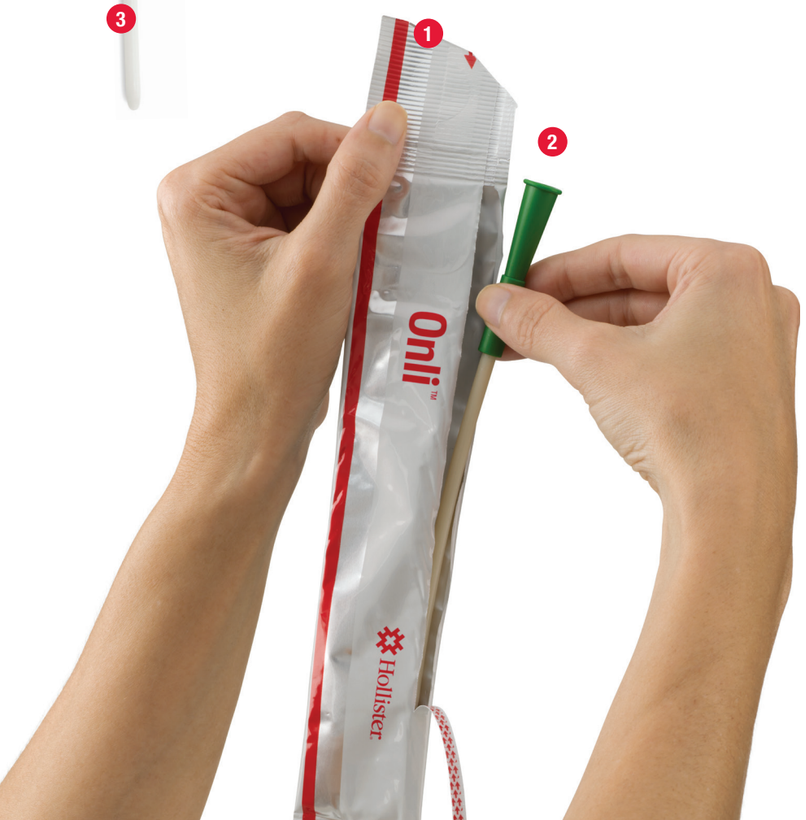

This intermittent catheter is a flexible tubular device that is inserted through the urethra by male, female and pediatric patients who need to drain urine from the bladder.

- Ready to use, single-use intermittent catheter
- Hydrophilic-coated, phthalate-free catheter
- 2 smooth catheter eyelets
- Color-coded funnel
- Not made with natural rubber latex

WARNING: To help reduce the potential for infection and/or other complications, do not reuse.

WARNING: If discomfort or any sign of trauma occurs, discontinue use immediately and consult your healthcare practitioner.

PRECAUTION: Please consult your healthcare practitioner before using this product if any of the following conditions are present: severed urethra, unexplained urethral bleeding, pronounced stricture, urethritis (inflammation of the urethra).

PRECAUTION: Self-catheterization should follow the plan of care and advice given by your healthcare practitioner and be carried out only in accordance with the instructions for use provided. Because catheterization frequency varies by person, the recommended frequency of your catheterization should be provided by your healthcare practitioner. For any other questions about your catheterization, please contact your healthcare practitioner.

CAUTION: Rx Only. Federal (USA) Law restricts this device to sale by or on the order of a physician or other healthcare practitioner licensed under state law to order this product. Prior to use of this device, be sure to read (i) the complete information on how to use this device including Warnings, Cautions, and Instructions for Use, and (ii) all other package inserts and labels supplied with the product.

NOTE: Store boxes in a flat position and at normal room temperature.

This product consists of: polyvinylchloride funnel and tubing not made with phthalates.

The Hollister logo and Onli are trademarks of Hollister Incorporated.
©2017 Hollister Incorporated.
923086-117

For detailed clinical questions concerning our products:
1.888.740.8999

For orders only:
1.800.323.4060

Hollister

Hollister Incorporated
Libertyville, IL USA

www.hollister.com

Onli

Ready for Use Hydrophilic Intermittent Catheter

Guide for Use

Whether your day is ordinary or extraordinary, the **Onli** catheter is there for you.

Designed to easily fit into your daily routine as a hassle-free and mess-free experience.


Ready. Simple.






Continence Care
People First

How the Urinary System Works

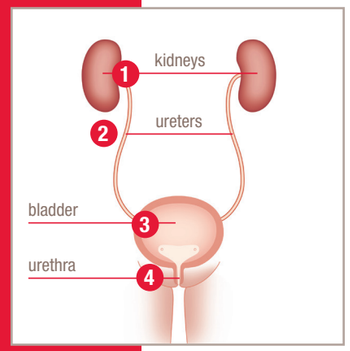

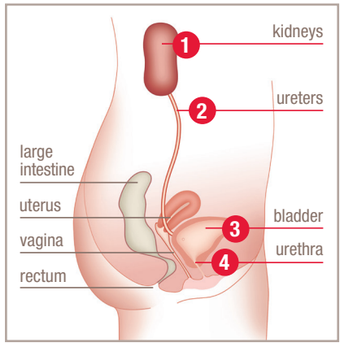

1 Urine is produced by the kidneys, which filter the waste products out of your body.

2 The liquid waste is passed via tubes called ureters to your bladder, the organ that stores urine.

3 When the bladder becomes full – a signal is sent to the brain to tell the urethral sphincter muscle to relax and the bladder to contract.


4 Urine flows down the urethra – the natural tube through which urine exits the bladder, and out of the body.

Self-Intermittent Catheterization (SIC)


When the bladder does not empty on its own, SIC may be recommended. Self-catheterization should be carried out under medical advice and only in accordance with instructions provided. It involves using a catheter to drain urine from your bladder via the urethra. Urine should be expelled on a regular basis throughout the day to keep the body healthy.




Wash hands with mild soap and water.

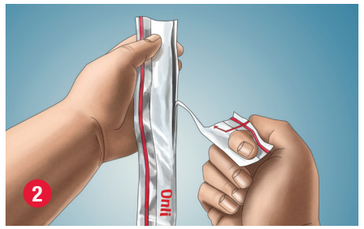


Open package by pulling the finger hole toward you.

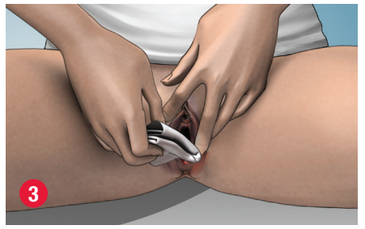

Spread the labia and cleanse around the opening of the urethra with mild, unscented soap or a non-alcoholic wet wipe.

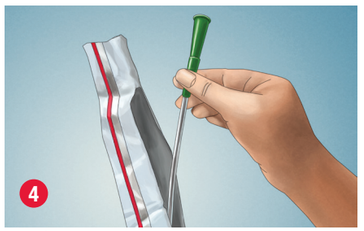


Hold funnel end to remove catheter from package.

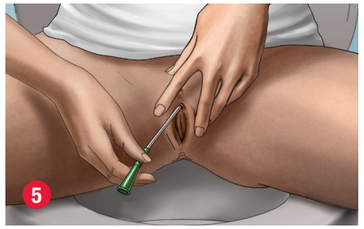

Spread labia with two fingers while inserting catheter into the urethra. Hold funnel, without touching the catheter and insert catheter until urine starts to flow.

Once urine flow has stopped, slowly withdraw the catheter to ensure bladder is completely empty. Gently remove catheter.

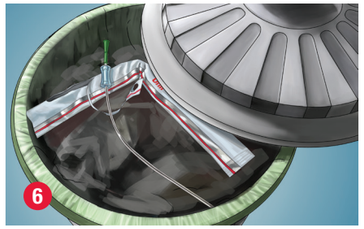

The catheter may be disposed in a waste bin. Do not flush catheter or package down the toilet.



Wash hands with mild soap and water.

Notes